

# Design and Development of an Experimental Setup to Study Tea Withering Process with Special Emphasis to RH and Temperature

Nipan Das<sup>1</sup>, Kunjalata Kalita<sup>2</sup>, P K Boruah<sup>3</sup> and Utpal Sarma<sup>4</sup>

<sup>1,2,3,4</sup>Dept. of Instrumentation & USIC, Gauhati University  
E-mail: <sup>1</sup>nipan.das86@yahoo.co.in

**Abstract**—In this paper, development of an instrumentation setup is reported for the study of tea withering process online. The parameters considered in this study are relative humidity (RH) and temperature at two different positions of the withering trough. Two sensor modules are installed to measure the temperature and relative humidity at the inlet and outlet of the airflow path. A load cell based weighing arrangement is also incorporated in the system for measuring the moisture loss in withering process by gravimetric method. A microcontroller based 10-bit resolution data acquisition system is incorporated to collect data in the process. Five sets of experiments are conducted and results are reported along with the correlation with the standard method of moisture loss i.e. gravimetric method or weight loss method. The observation shows a considerable change in the difference in variation of temperature and relative humidity at the inlet and outlet of airflow path in the withering trough during the process of withering. The design considerations of a scaled down prototype of a withering trough and the associated signal conditioning of the sensors are reported in the paper.

## 1. INTRODUCTION

Tea is one of the most popular beverages. Moisture measurement plays an important role in the manufacturing process of tea. The quality and durability of produced tea is highly dependent upon the proper level of moisture in the processing steps involved in the manufacturing of tea. The quality of intermediate processing depends not only on the moisture level of the current process, but also on the moisture levels of previous. Hence, it is very important to measure and maintain proper level of moisture content in tea manufacturing process.

Withering is the foundation for achieving quality in tea manufacture and the first processing step (in the factory) in which freshly plucked leaf is conditioned physically, as well as, chemically for subsequent processing stages. The chemical withering (starts immediately after plucking) contributes to the quality attributes of tea like the 'body' and 'flavour' [1]. The impact of withering in the quality of the final product is always an important aspect. Tombs K. I. & Mashingaidze A. reported the influence of withering, including leaf handling,

on the manufacturing and quality of black teas [2]. Soheilifard Farshad et al. studied the impact of time in withering for some biochemical properties and sensory quality attribute in final product [3]. Baruah D. et al. reported that chemical wither for a longer period produces liquor with better flavor quality and fuller cup characters [4]. Various biochemical processes that occurs during withering of black tea production is reported by Omiadze N. T. et al. [5].

The physical withering reduces the moisture content of the fresh leaf which ranges between 74% – 83% and correct withering is essential for quality, although, it has always been a difficult task to determine the end-point of withers. The physical withering also makes the leaf 'flaccid' or 'rubbery' which is essential for the subsequent steps of processing. The same reduction in moisture percentage and increase of flaccidity of leaf to the desired level can be achieved in a shorter period but a longer period is (normally takes about 12 – 16 hours) necessary for chemical wither. Therefore, physical wither is regulated at a slower rate, so as to reach the desired physical withering in the same interval as required for the chemical wither. The objectives are achieved by passing air through the leaves [1].

Due to various advantages, trough withering is the most popular system currently being used all over the world. The troughs are of two types – (a) Open trough and (b) Enclosed trough [6]. However, attempts are going on for improvement of trough such as one reported by Singh Divya et al. [7].

In withering process, the drying is accomplished by vaporizing the water (moisture) contained in the tea leaves; and to do this the latent heat of vaporization must be supplied. There are two important process-controlling factors that enter into the unit operation of drying:

- a) Transfer of heat to provide the necessary latent heat of vaporization,





The residual plot is shown in Fig. 6.

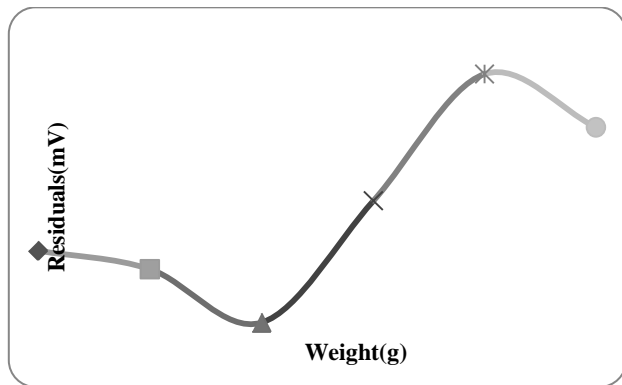


Fig. 6: Residual plot for weighing system calibration

### 3.3 Data Acquisition

The outputs of two pairs of sensors are connected to 4 channels of inbuilt ADC (Analog to digital converter) of an ATmega8 [21] microcontroller. The output voltage (Vout3) from the load cell signal conditioning circuit is connected to one ADC channel of another ATmega8 microcontroller. The two microcontrollers are connected to a PC (Personal Computer) by RS485 network. An algorithm is developed for reading the sensors, compensating the effect of temperature in RH measurement and finally sending the data to PC in proper format. The developed algorithm is implemented in ATmega8 microcontroller by writing suitable C-code in Atmel Studio4 IDE (Integrated Development Environment) [22]. The temperature compensation is done using the equation (1& 2). To log the received data in a PC, a program is developed in C language using Turbo C++ IDE. Data are stored in PC in .XLS format along with records of date and time. Fig. 7 & Fig. 8 show the flowchart of developed algorithms that are implemented in microcontroller and PC respectively.

The added network capability to the ATmega8 microcontroller boards enables the extensibility of the system to be used for more number of sensors in a bigger trough.

## 4. EXPERIMENTAL RESULTS

In the prototype of the trough, fresh tea leaves are loaded on the withering bed. The withering process was started by running the fan at a constant speed of air flow rate (AFR) of  $0.25\text{m}^3/\text{s}$ . The process is continued at ambient temperature and RH. The data acquisition system is employed to record the data continuously at an interval of 7 seconds for all the sensors (including load cell) along with the records of date and time.

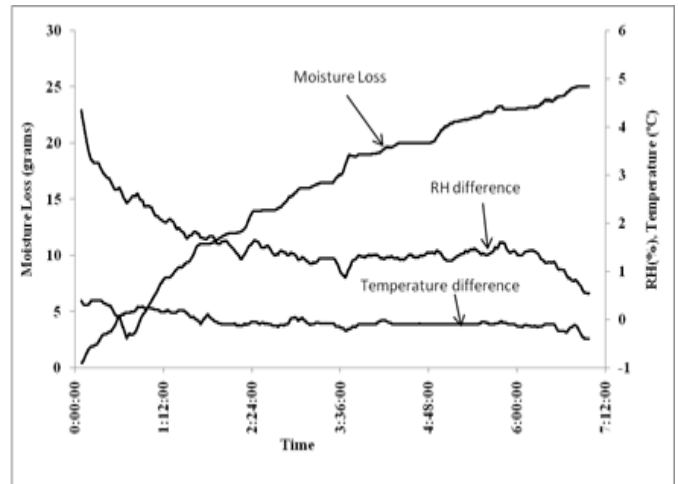


Fig. 7: Test 1 shows the moisture loss obtained from gravimetric method and difference of RH and Temperature at inlet and outlet of airflow path of the withering trough.

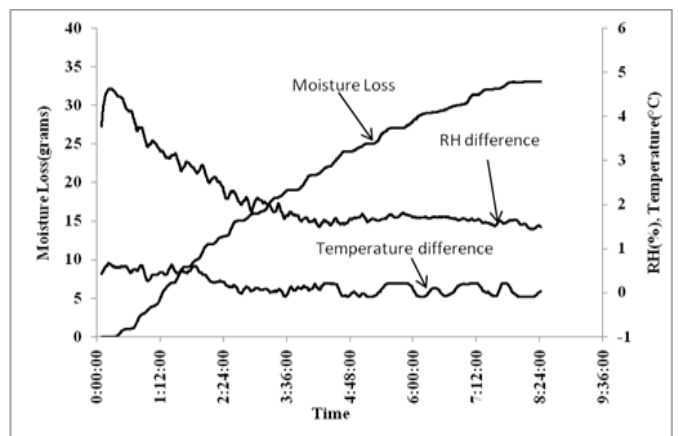


Fig. 8: Test 2 shows the moisture loss obtained from gravimetric method and difference of RH and Temperature at inlet and outlet of airflow path of the withering trough.

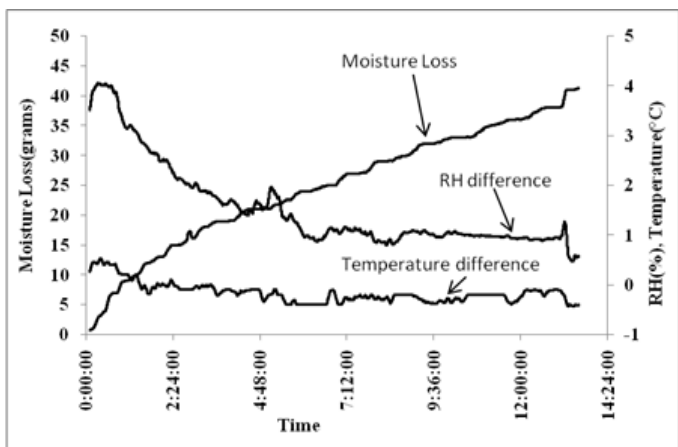


Fig. 9: Test 3 shows the Moisture loss obtained from weight loss method and difference of RH and Temperature at inlet and outlet of airflow path of the withering trough

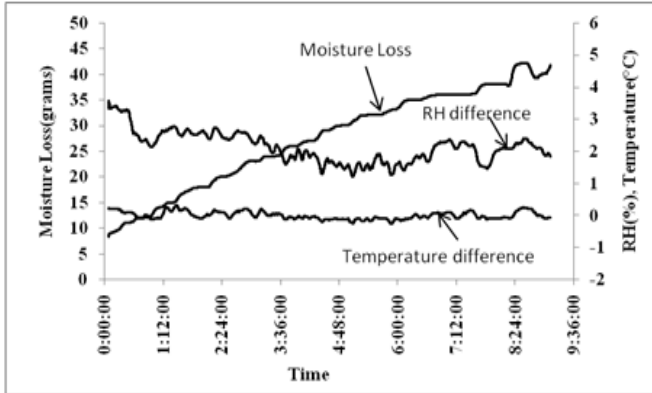


Fig. 10: Test 4 shows the Moisture loss obtained from weight loss method and difference of RH and Temperature at inlet and outlet of airflow path of the withering trough.

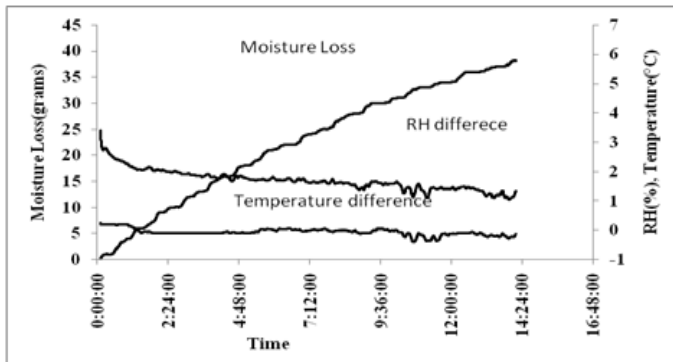


Fig. 11: Test 5 shows the Moisture loss obtained from weight loss method and difference of RH and Temperature at inlet and outlet of airflow path of the withering trough.

Experimental results are shown in table 1.

Table 1

Experi- ment No.	Loaded leaf weight (grams)	Withering time (hh.mm)	Maxim- um RH differen- ce	Minimum RH difference	Moisture loss (grams)
1	76	7	5.1%	0.5 %	25
2	89	8.30	4.8%	1.2 %	33
3	89	13.30	4.2%	0.3 %	42
4	103	9.05	5.5%	1.7 %	42
5	113	14.10	6.3%	0.8 %	39

In all these experiments temperature at inlet is higher compared to outlet by 0.7°C (±0.1°C) and outlet temperature gradually increases and becomes higher than the inlet by 0.4°C (±1°C).

At the initial stage of withering process the difference of RH at outlet and inlet is less and even sometimes inlet RH is more compared to outlet RH. This is due to the random distribution

of moisture in the surroundings of the bed and accumulation of moisture in the chamber of withering trough. After the removal of accumulated moisture from the trough chamber the actual withering starts. It takes around 10 minutes to remove the accumulated moisture from the chamber.

## 5. CONCLUSION AND DISCUSSION

The developed instrumentation for the measurement of RH and temperature are designed as modular nodes. The network capability of the nodes provide extensibility and applicability of the system in an actual trough. There is also possibility to configure the nodes as smart sensors.

Five experiments are carried out in a scaled down prototype of actual withering trough and in one directional airflow path i.e. one dimensional mass flow. The experimental results show that RH at the outlet is more compared to inlet in the air flow path. That means the moving air carries the moisture from tea leaves towards the outlet. Again the temperature at outlet is less compared to the inlet of airflow path in all the five experiments.

Since a considerable difference in RH and temperature is obtained at the inlet and outlet of the airflow path, from further investigation moisture loss can be measured from the measurement of RH and temperature at the inlet and outlet. Again proper investigation of theoretical approach or employment of soft computing tool can give better prediction of moisture loss in the withering process. For implementing the system in factory, consideration of some new parameters may be necessary.

Since online monitoring of moisture loss in withering is always been a problem in withering process. The developed system can provide a solution for the problem, that usually faced by the tea factory, without disturbing the current setup of withering troughs.

## REFERENCES

- [1] <http://www.tocklai.net/activities/tea-manufacture/withering/>
- [2] K. I. Tombs & A. Mashingaidze, "Influence of withering, including leaf handling, on the manufacturing and quality of black teas - a review", Food Chemistry, Vol. 60, No. 4, pp. 573-580, 1997, Elsevier Science Ltd.
- [3] Farshad Soheili-Fard, Hamid Reza Ghassemzadeh and Seyed Babak Salvatian, "Impact of Withering time duration on some Biochemical Properties and Sensory Quality Attributes of Black Tea", Biological Forum – An International Journal 7(1): 1045-1049(2015)
- [4] D. Baruah, L. P. Bhuyan, M. Hazarika, "Impact of moisture loss and temperature on biochemical changes during withering stage of black tea processing on four Tocklai released clones", Two and a Bud 59(2): 134-142, 2012.
- [5] N. T. Omiadzea, N. I. Mchedlishvilia, J. N. Rodriguez\_Lopezb, M. O. Abutidzea, T. A. Sadunishvilia, and N. G. Pruidzea, "Biochemical Processes at the Stage of Withering during Black

- Tea Production” Applied Biochemistry and Microbiology, 2014, Vol. 50, No. 4, pp. 394–397. Pleiades Publishing, Inc., 2014.
- [6] K.C. Wilson, M.N. Clifford, “Tea: Cultivation to consumption”, First edition 1992, Springer Science+Business Media, ISBN 978-94-01 0-5027-2 0 442 231419 1(USA)
- [7] Divya Singh, Tanmoy Samantal, Shrilekha Das, A. K. Ghosh, A. Mitra and B. C. Ghosh, “Development of a customized trough to study withering of tea leaves”, Two and a Bud 59(2):143-147, 2012
- [8] Chistie J. Geankplis, “Transport Processes and Unit Operations”, Third Edition, Prantice-Hall international, Inc., 1993.
- [9] Manabendra Bhuyan, “Measurement and Control in Food Processing”, Taylor & Francis, 2007.
- [10] Seichi Okamura, Yangjun Zhang and Nobuhito Tsukamoto, “A new microstripline-type moisture sensor for heavily wet tea leaves”, Meas. Sci. Technol. 18 (2007) 1022–1028.
- [11] D. Hazarika, S. Laskar, A. Sarma, and P. K. Sarmah, “PC-Based Instrumentation System for the Detection of Moisture Content of Tea Leaves at Its Final Stage”, IEEE transactions on Instrumentation and Measurement, vol. 55, no. 5, october 2006.
- [12] H. M. Ghodake, T. K. Goswami, and A. Chakraverty, “Mathematical Modeling of Withering Characteristics of Tea Leaves”, Drying Technology, 24: 159–164, 2006.
- [13] W.S. Botheju, K.S.P. Amarathunge and I.S.B. Abeysinghe, “Simulation of Trough Withering of Tea using One Dimensional Heat and Mass Transfer Finite Difference Model”, Tropical Agricultural Research Vol. 22 (3): 282 - 295 (2011).
- [14] Andrew Chen, Hsuan-Yu Chen and Chiachung Chen, “Use of Temperature and Humidity Sensors to Determine Moisture Content of Oolong Tea”, *Sensors* 2014, 14, 15593-15609; doi:10.3390/s140815593
- [15] Datasheet of LM35, [www.ti.com/lit/ds/symlink/lm35.pdf](http://www.ti.com/lit/ds/symlink/lm35.pdf)
- [16] Datasheet of HCH5030, [sensing.honeywell.com/index.php?ci\\_id=49692](http://sensing.honeywell.com/index.php?ci_id=49692)
- [17] Datasheet of MCP1525/41, [ww1.microchip.com/downloads/en/DeviceDoc/21653b.pdf](http://ww1.microchip.com/downloads/en/DeviceDoc/21653b.pdf)
- [18] Datasheet of TLC272, [www.ti.com/lit/ds/symlink/tlc272.pdf](http://www.ti.com/lit/ds/symlink/tlc272.pdf)
- [19] Datasheet of LM336-2.5, [www.ti.com.cn/cn/lit/ds/symlink/lm336-2.5-n.pdf](http://www.ti.com.cn/cn/lit/ds/symlink/lm336-2.5-n.pdf)
- [20] Datasheet of AD620, [www.analog.com/media/en/technical-documentation/data.../AD620.pdf](http://www.analog.com/media/en/technical-documentation/data.../AD620.pdf)
- [21] Datasheet of ATmega8, [www.atmel.com/.../Atmel-2486-8-bit-AVR-microcontroller-ATmega8\\_L...](http://www.atmel.com/.../Atmel-2486-8-bit-AVR-microcontroller-ATmega8_L...)  
[www.atmel.com/tools/ATMELSTUDIO.aspx](http://www.atmel.com/tools/ATMELSTUDIO.aspx)